



How to correct “white balance” Parameter



1. Operate AWC , wait 5 seconds , then go next step

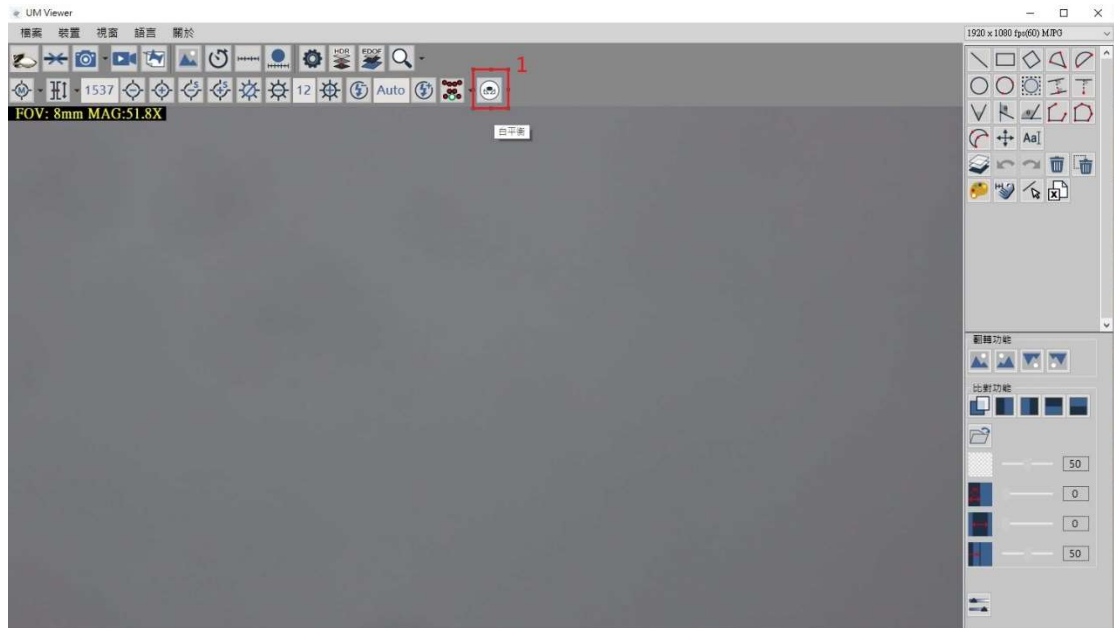


2. Open Video Setting

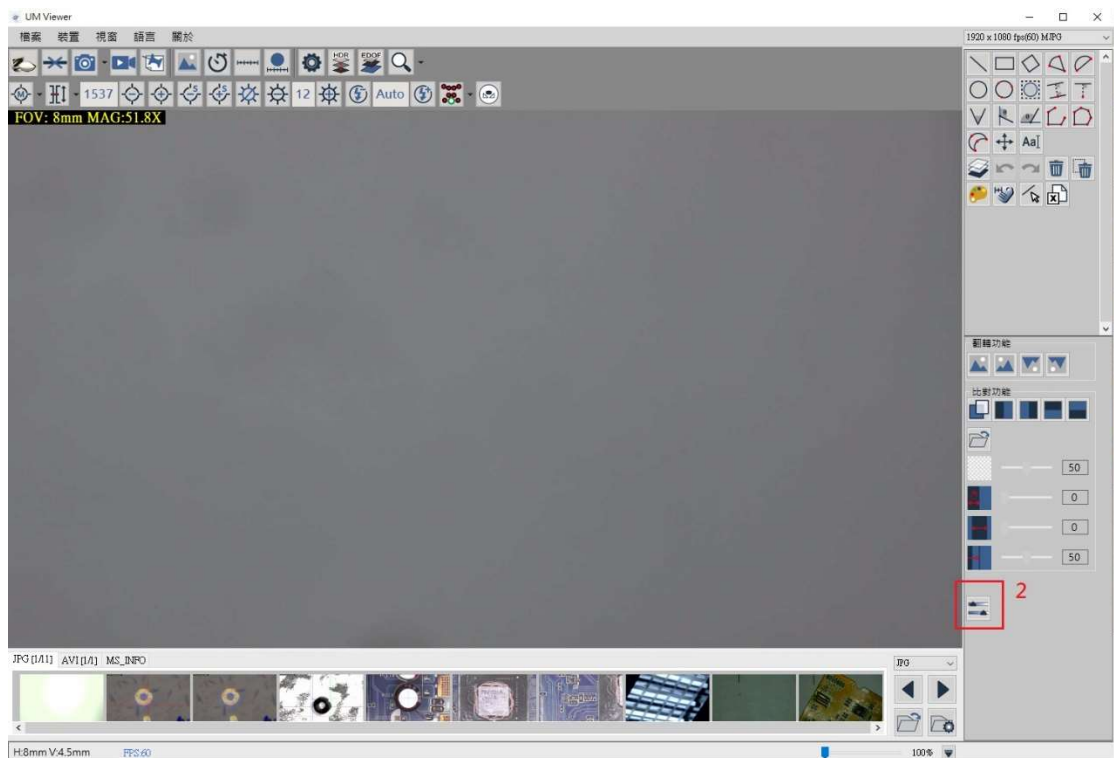


3. Uncheck AWB automatically

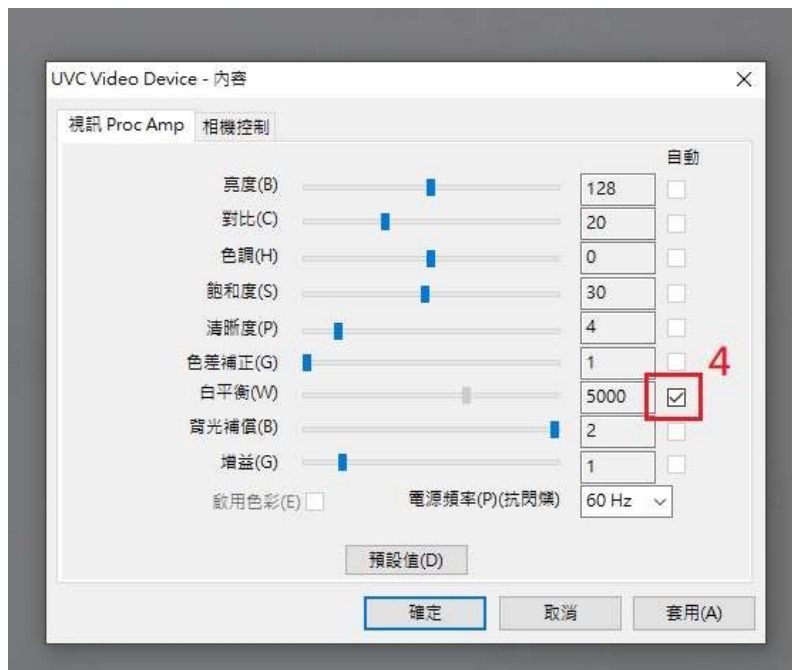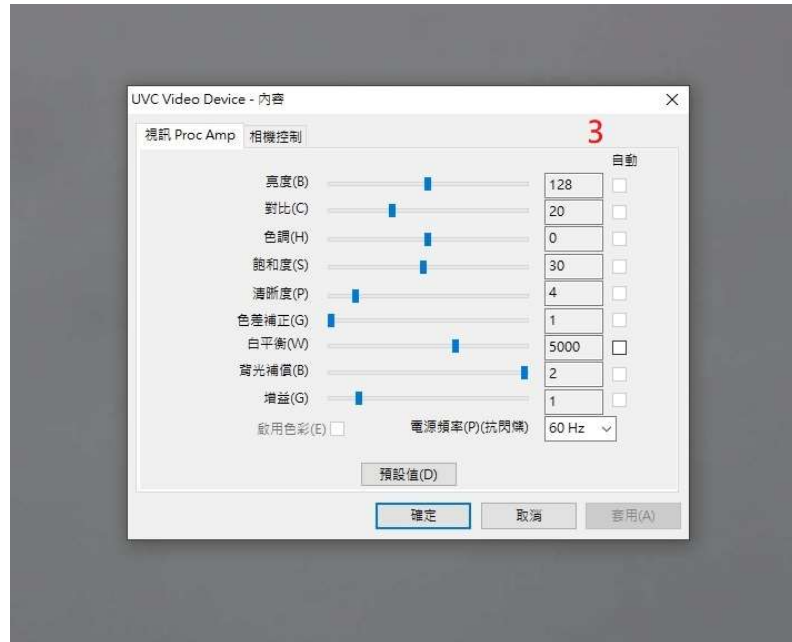


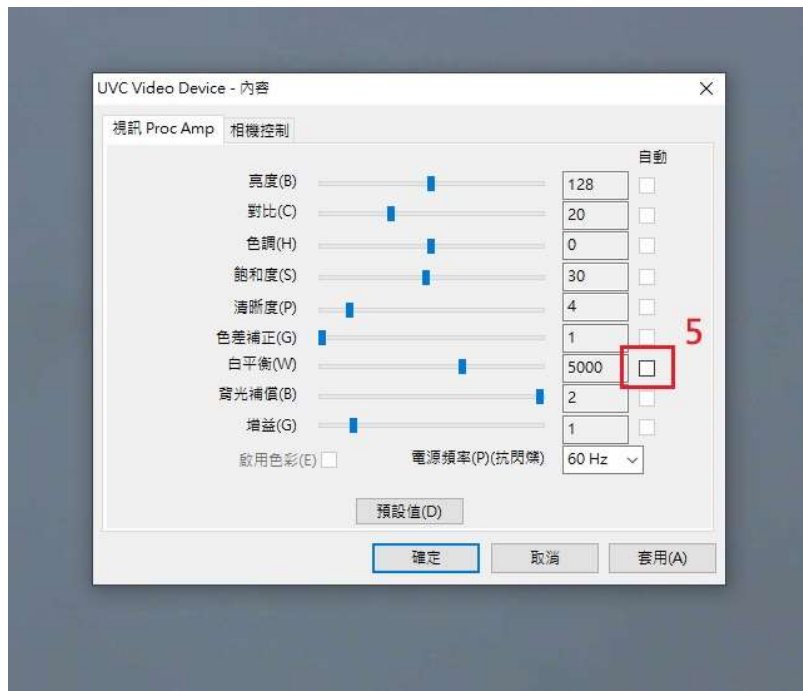


4. Pull BAR back and forth (e.x. 5000->5100->5000)

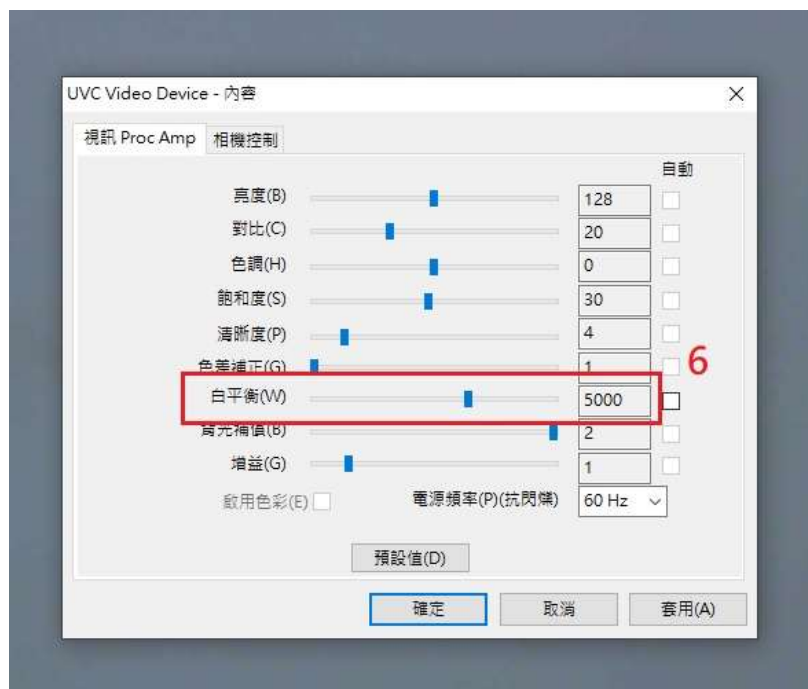

5. Press “confirmed” finally

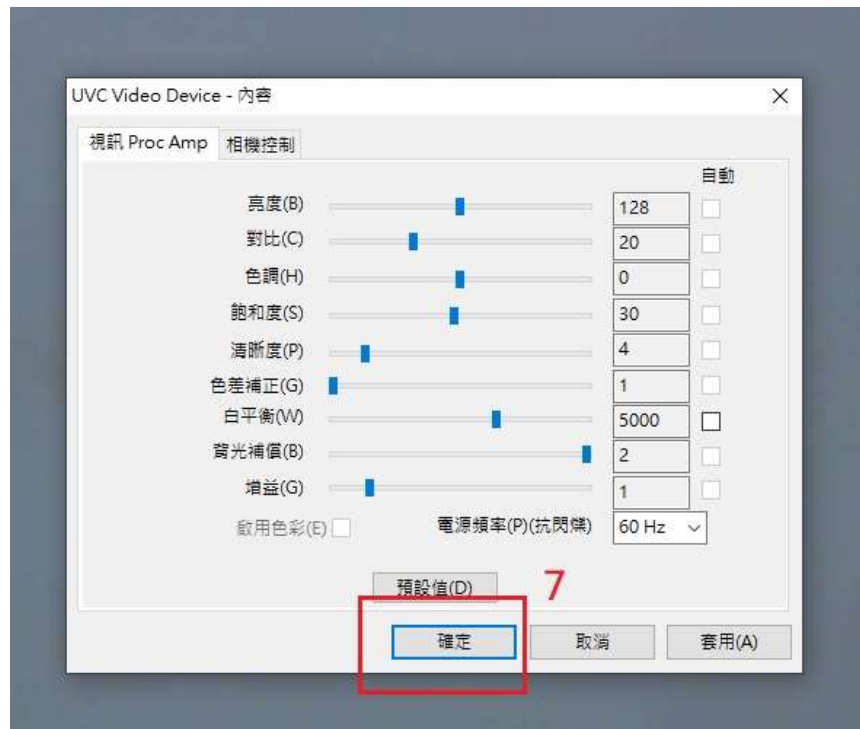

6. Off line

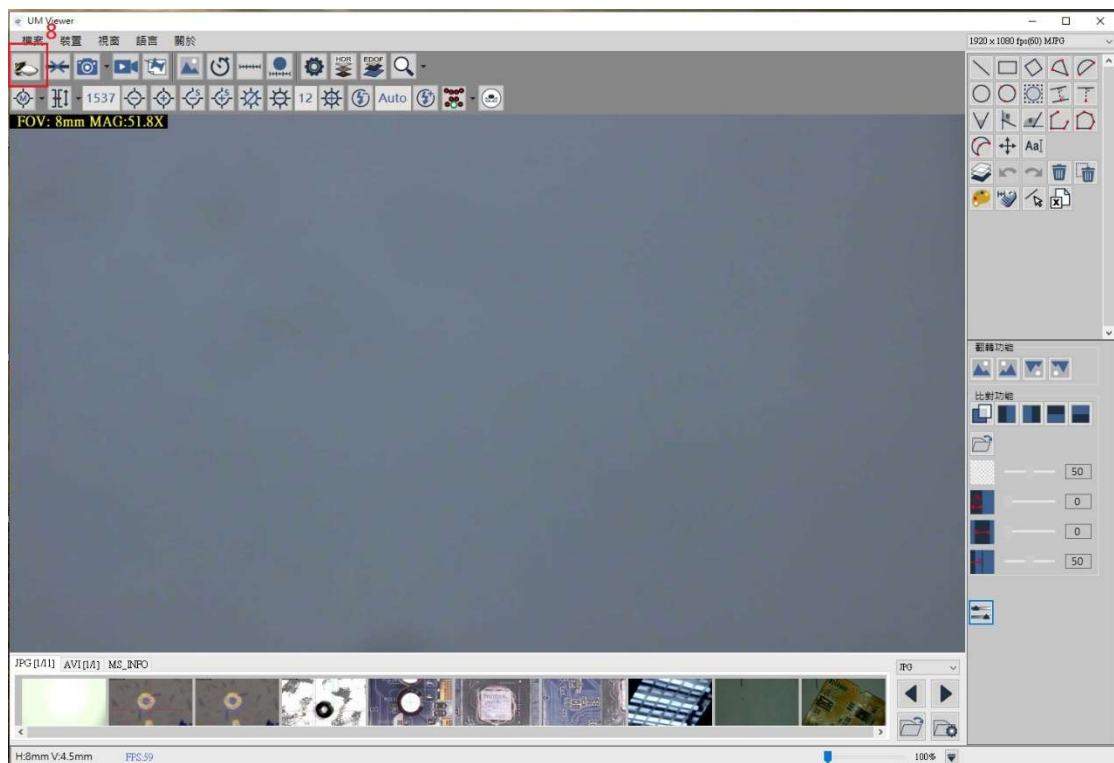

7. Unplug the microscope